


モノクローナル抗体混合物のオンラインネイティブ質量分析(HIC-MS)

Online native HIC-MS analysis of a monoclonal antibody mixture

W200519A

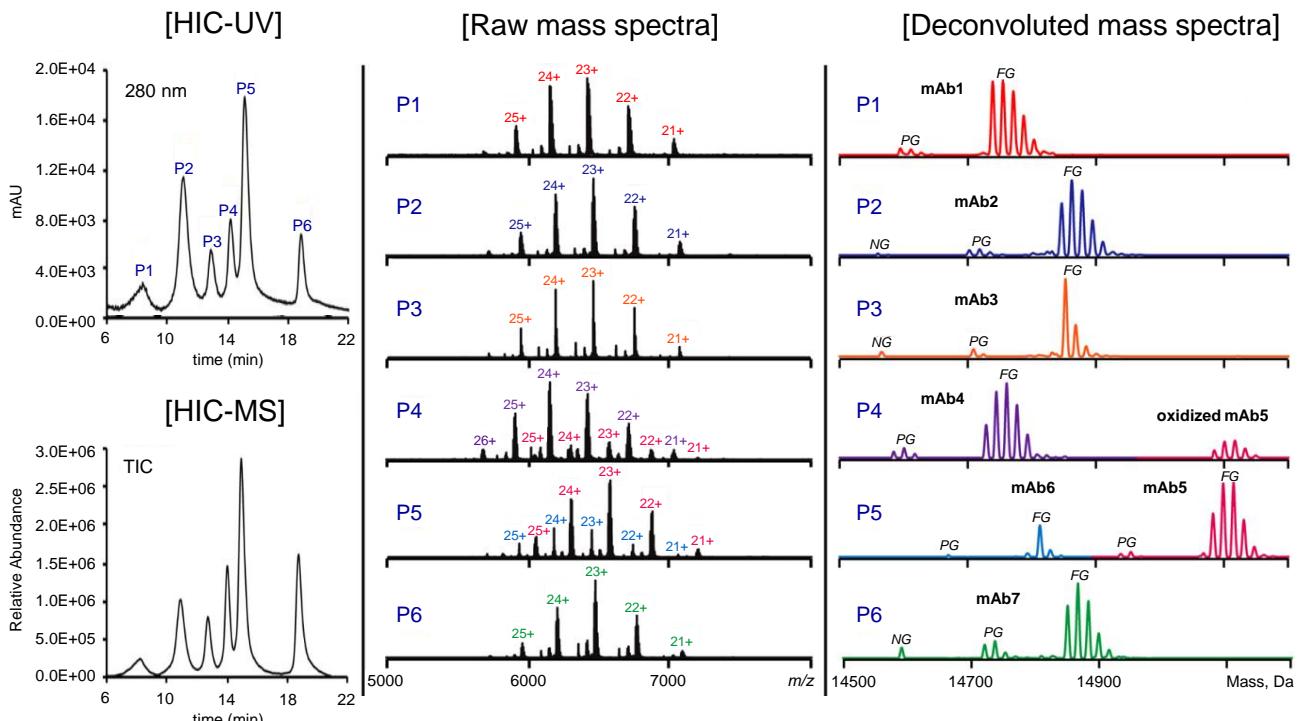

Courtesy of S. Wang, Regeneron Pharmaceuticals Inc.

Column	: BioPro HIC BF (4 μ m) 100 X 4.6 mmI.D.
Eluent	: A) 3 M $\text{CH}_3\text{COONH}_4$ B) water 0% B (0-2 min), 0-90% B (2-18 min), 90% B (18-22 min)
Flow rate	: 0.3 mL/min (To enable online simultaneous UV and MS detection, a post-column makeup and splitting flow platform was applied.)
Temperature	: ambient
Detection	: UV at 280 nm, nanospray ionization-mass spectrometry (NSI-MS)
Injection	: 3 μ L
Sample	: A mixture of seven different in-house mAbs (1-2 mg/mL each)
System	: LC) Ultimate TM 3000 UHPLC system (Thermo Fisher Scientific) MS) Q Exactive TM UHMR mass spectrometer (Thermo Fisher Scientific)

Reference:

Y. Yan, T. Xing, S. Wang, T. J. Daly, N. Li, Online coupling of analytical hydrophobic interaction chromatography with native mass spectrometry for the characterization of monoclonal antibodies and related products, J. Pharm. Biomed. Anal. 186 (2020) 113313.