

ブデソニド（米国薬局方記載条件）



Budesonide (The United State Pharmacopeia)

P220324D

	System suitability requirement	Result
Resolution (1,2)	≥1.2	1.9
Relative standard deviation for the sum of the peak areas of the two budesonide epimers (n=5)	≤1.0%	0.053%

mAU

1. Epimer B of Budesonide
2. Epimer A of Budesonide

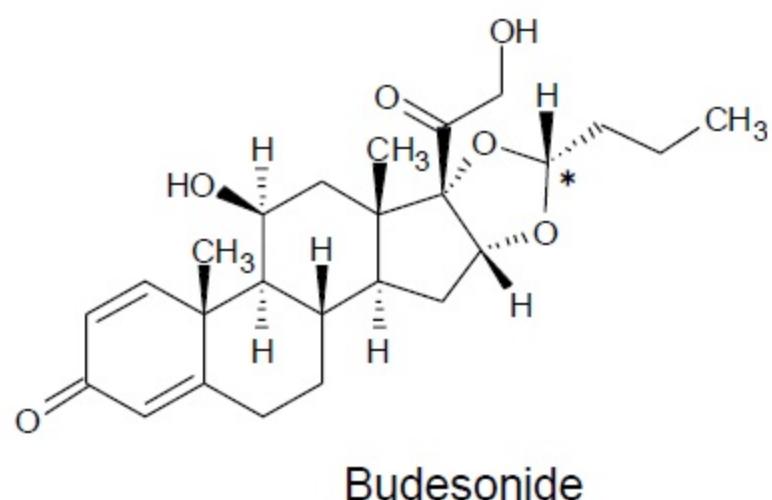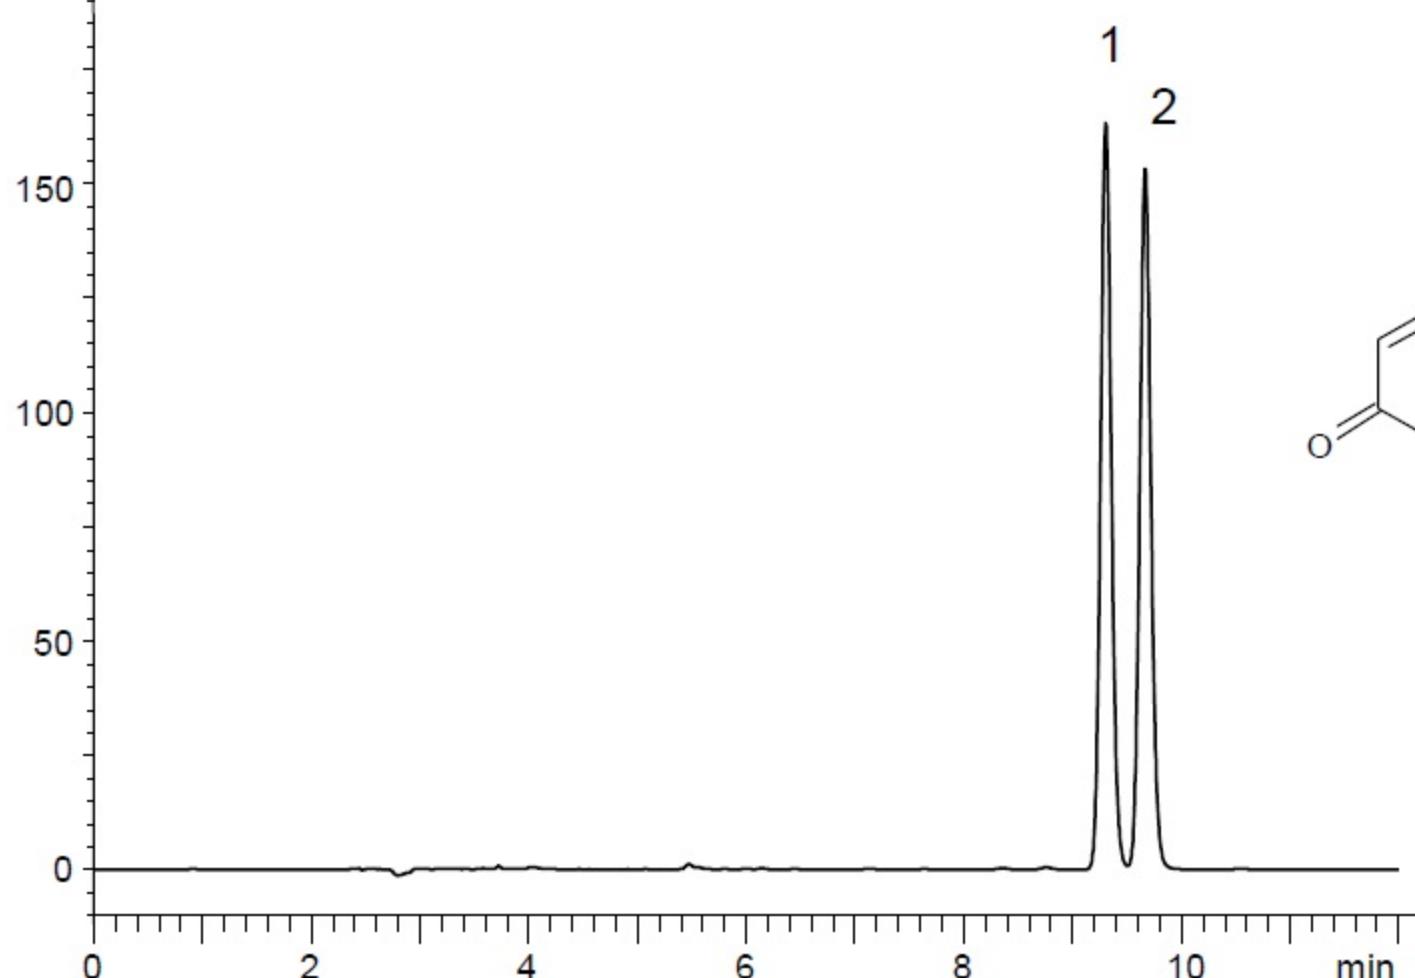

Column	: YMC-Pack ODS-A (3 µm, 20 nm) 250 X 4.6 mmI.D.
Eluent	: buffer (pH 3.9)*1/acetonitrile (55/45) <small>*1 0.5 mL of glacial acetic acid in 1 L of water, adjust pH 3.9 with KOH</small>
Flow rate	: 1.0 mL/min
Temperature	: 50°C
Detection	: UV at 240 nm
Injection	: 20 µL
(The United State Pharmacopeia 42nd; Assay)	

*2 Standard solution was prepared from Budesonide supplied as a reagent for laboratory use.